



COUPLED TANKS

Installation & Commissioning

33-041-IC

(For use with MATLAB
R2007a or later)

Feedback Instruments Ltd., Park Road, Crowborough, East Sussex, TN6 2QR, UK
Telephone: +44 (0) 1892 653322, Fax: +44 (0) 1892 663719
E-mail: feedback@feedback-instruments.com, Website: www.feedback-instruments.com

Manual: 33-041-IC Ed02 042009
Feedback Part No. 1160-33041IC

THE HEALTH AND SAFETY AT WORK ACT 1974

We are required under the Health and Safety at Work Act 1974, to make available to users of this equipment certain information regarding its safe use.

The equipment, when used in normal or prescribed applications within the parameters set for its mechanical and electrical performance, should not cause any danger or hazard to health or safety if normal engineering practices are observed and they are used in accordance with the instructions supplied.

If, in specific cases, circumstances exist in which a potential hazard may be brought about by careless or improper use, these will be pointed out and the necessary precautions emphasised.

While we provide the fullest possible user information relating to the proper use of this equipment, if there is any doubt whatsoever about any aspect, the user should contact the Product Safety Officer at Feedback Instruments Limited, Crowborough.

This equipment should not be used by inexperienced users unless they are under supervision.

We are required by European Directives to indicate on our equipment panels certain areas and warnings that require attention by the user. These have been indicated in the specified way by yellow labels with black printing, the meaning of any labels that may be fixed to the instrument are shown below:



CAUTION -
RISK OF
DANGER



CAUTION -
RISK OF
ELECTRIC SHOCK



CAUTION -
ELECTROSTATIC
SENSITIVE DEVICE

Refer to accompanying documents

PRODUCT IMPROVEMENTS

We maintain a policy of continuous product improvement by incorporating the latest developments and components into our equipment, even up to the time of dispatch.

All major changes are incorporated into up-dated editions of our manuals and this manual was believed to be correct at the time of printing. However, some product changes which do not affect the instructional capability of the equipment, may not be included until it is necessary to incorporate other significant changes.

COMPONENT REPLACEMENT

Where components are of a 'Safety Critical' nature, i.e. all components involved with the supply or carrying of voltages at supply potential or higher, these must be replaced with components of equal international safety approval in order to maintain full equipment safety.

In order to maintain compliance with international directives, all replacement components should be identical to those originally supplied.

Any component may be ordered direct from Feedback or its agents by quoting the following information:

1. Equipment type
2. Component reference
3. Component value
4. Equipment serial number

Components can often be replaced by alternatives available locally, however we cannot therefore guarantee continued performance either to published specification or compliance with international standards.

CE DECLARATION CONCERNING ELECTROMAGNETIC COMPATIBILITY

Should this equipment be used outside the classroom, laboratory study area or similar such place for which it is designed and sold then Feedback Instruments Ltd hereby states that conformity with the protection requirements of the European Community Electromagnetic Compatibility Directive (89/336/EEC) may be invalidated and could lead to prosecution.

This equipment, when operated in accordance with the supplied documentation, does not cause electromagnetic disturbance outside its immediate electromagnetic environment.

COPYRIGHT NOTICE

© **Feedback Instruments Limited**

All rights reserved. No part of this publication may be reproduced, stored in a retrieval system, or transmitted, in any form or by any means, electronic, mechanical, photocopying, recording or otherwise, without the prior permission of Feedback Instruments Limited.

ACKNOWLEDGEMENTS

Feedback Instruments Ltd acknowledge all trademarks.

MATLAB is a registered trademark of Mathworks Inc.

Table of Contents

Manual overview	1
Required manuals and equipment	2
Packing List	3
Unit assembly	4
Advantech PCI1711 card installation guide.....	6
Installing from a CD – new installation	6
Upgrading and installing downloaded files	15
Coupled Tanks System software installation.....	18
PC and Coupled Tanks connection.....	22
Location of Simulink model files	23
Sensor calibration.....	25
Coupled Tanks Mechanical Unit description.....	28
Computer control	33
Simulink Coupled Tanks control.....	35
Real-time control	35
New controllers design	37
<i>PCI 1711 Lab I/O Block – Feedback DAC</i>	<i>38</i>

MANUAL OVERVIEW**Manual overview**

This manual serves as a set of installation instructions for the Coupled Tanks Setup. Firstly, it explains which elements belong to the setup and how they are connected. The software installation process is described, and finally the details of how the Coupled Tanks System is controlled with the PC in the Matlab environment are presented. Precautions are underlined.

Required manuals and equipment

The following equipment and manuals are required for the use of the Coupled Tanks System:

- 1 PC with Windows 2000 or Windows XP
- 2 Matlab V7.4 (R2007a) or later with Simulink
- 3 Matlab Toolboxes:
 - Real Time Workshop with Real Time Windows Target
 - System Identification Toolbox (necessary to perform identification exercises)
 - Control Toolbox (necessary to perform controller synthesis)
- 4 Advantech PCI1711 card
- 5 Coupled Tanks – Mechanical and Electronic Units
- 6 Software installation CDs
- 7 '*Installation & Commissioning*' manual
- 8 '*Control Experiments*' manual
- 9 '*Matlab Guide*' manual

The following equipment is supplied by Feedback Instruments as 33-041 (Coupled Tanks System):

- 1 33-230 - Coupled Tanks rig with Software Pack
- 2 Advantech PCI card with cables and connector box

Packing List

Unpack the items and remove all packing and securing material. Apart from software installation CD's you should have the following items:

- 1) 33-230 – Coupled Tanks rig with Tanks and Pumps mounted
- 2) 1 SCSI cable
- 3) Connector box
- 4) LPT 25 way cable

Unit assembly

Connect the unit according to Figure 1 and the following instructions.

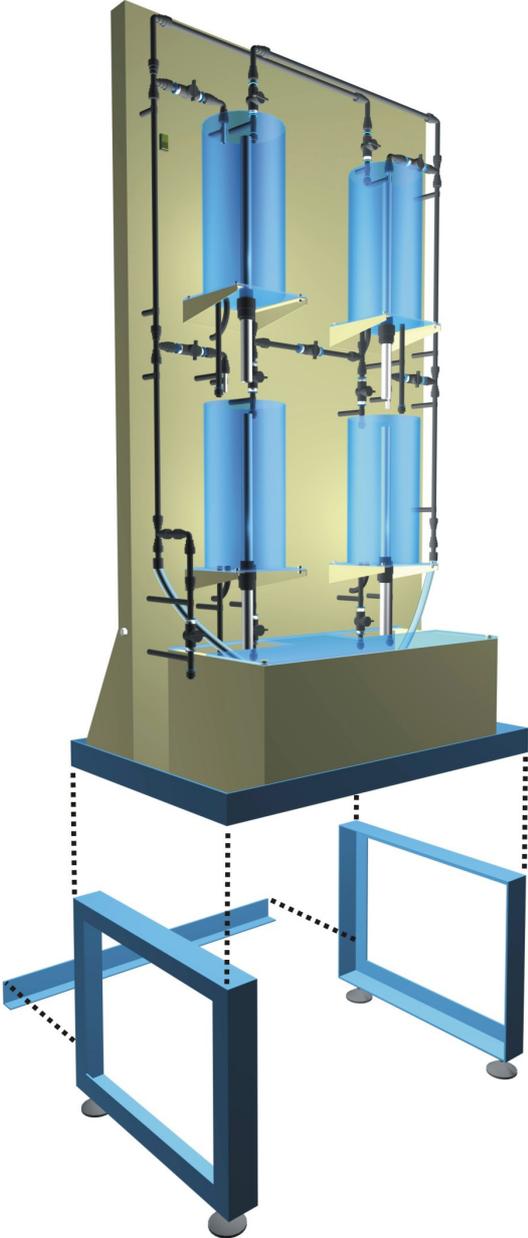


Figure 1 Assembled Coupled Tanks unit

- Assemble the bottom stand for the Coupled Tanks if necessary. Use the supplied screws to attach the legs to the rig.

Advantech PCI1711 card installation guide

It is assumed that a PC is available with Matlab, Simulink, Real-Time Workshop and Real-Time Windows Target correctly installed and functioning.

During the installation of the Advantech PCI-1711 card make sure you follow the instructions given in this section. This will ensure that common installation problems are avoided.

You must have administrator privileges on the PC before you can carry out this software installation.

Install the software supplied with the PCI-1711 card first. The PCI-1711 card must not be installed until the driver software has been installed correctly. A PCI-1711 device driver version 2.2 or higher is recommended.

Installing from a CD – new installation

Ensure that you have the latest drivers (Universal 32-bit DLL Drivers V2.2 and device manager V2.4). If not, download the files from the Advantech website and refer to the procedure above for installation.

1. Insert the CD supplied with the PCI-1711 card into the PC. The installation programme will automatically start. The following window will open (Figure 2).



Figure 2 Initial Installation Window

2. Press 'CONTINUE' to enter the installation menu (Figure 3).



Figure 3 Installation Menu

3. To install the software select 'Installation'. The following window will appear (Figure 4)



ADVANTECH PCI1711 CARD INSTALLATION GUIDE
Figure 4 Installation Element Selection Window

4. Select 'Device Manager'. The following window will open (Figure 5).



Figure 5 Device Manager Installation Window

5. Press 'Next' to continue to the License Agreement window presented in Figure 6.



ADVANTECH PC1711 CARD INSTALLATION GUIDE

Figure 6 License Agreement Window

6. Read the terms of the license agreement and press 'Yes' if you accept. The User information window will appear (Figure 7).



Figure 7 User Information Window

- Fill the fields with proper information and press 'Next'. The Destination Folder information window will appear (Figure 8).



Figure 8 Destination Folder Window

- Choose the destination folder and press 'Next'. The Setup Type information window will appear (Figure 9).



Figure 9 Setup Type Window

9. Select the Typical Setup and press 'Next'. The Program Folder information window will appear (Figure 10).



Figure 10 Program Folder Selection Window

10. Select the Program Folder and click 'Next' to proceed. The setup information window will appear. Click 'Next' to continue the setup. The necessary files will be copied and the Device Manager installation will finish.
11. Return to the main installer menu (Figure 4). To install the card driver select 'Individual Driver'. The menu appears as shown in Figure 11.

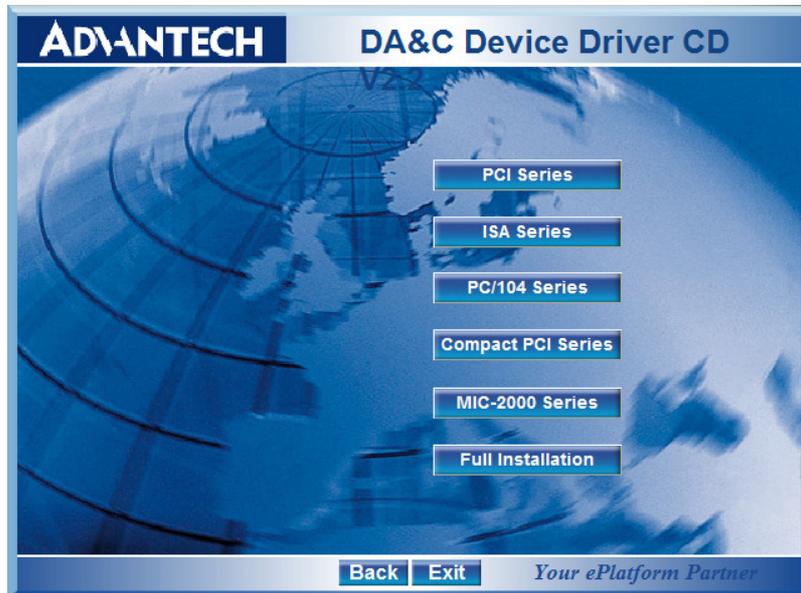


Figure 11 Main Menu

ADVANTECH PCI1711 CARD INSTALLATION GUIDE

12. Select the 'PCI Series'. The card choice window will open (Figure 12).

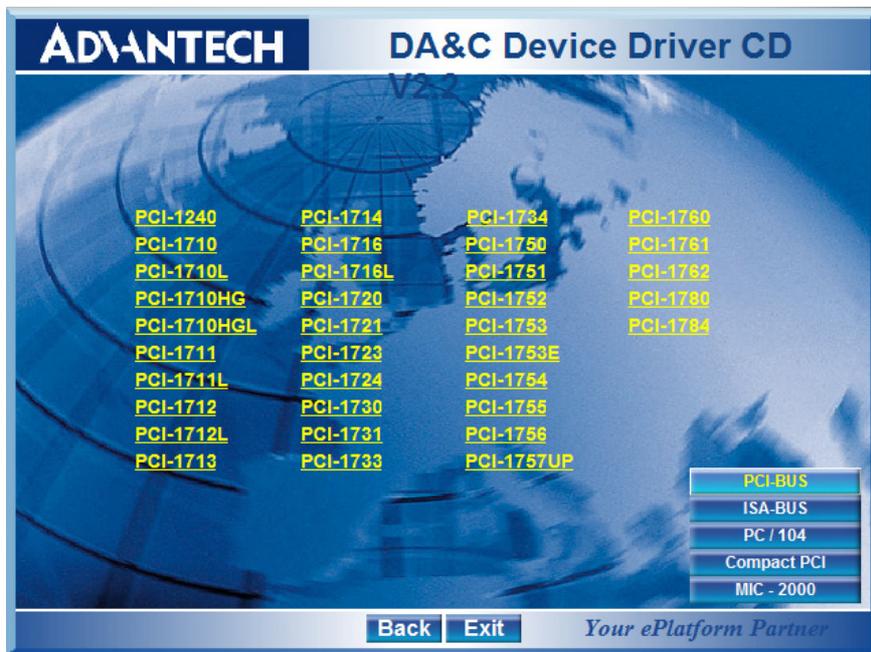


Figure 12 Card Choice Menu

13. Select the 'PCI-1711'. The driver installer will open in a new window (Figure 13).



Figure 13 PCI-1711 Driver Installation Window

14. Click 'Next' to proceed. Select the Typical installation (Figure 14) and click 'Next' to continue to the setup information window.

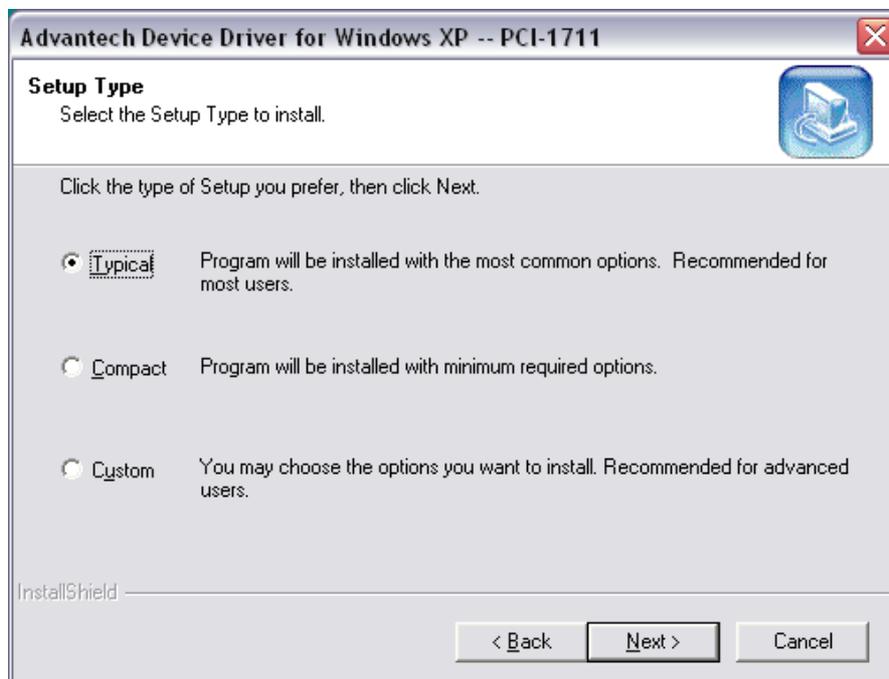


Figure 14 Setup Type Window

15. Click 'Next' to proceed with the installation. The necessary files will be copied and the installer will finish.
16. Turn the PC off and use any free PCI slot to insert the PCI-1711 into. Restart the PC. During the start up Windows will automatically install the driver for the PCI-1711.
17. To check that the card has installed correctly, navigate from the Start → All Programs menu to Advantech and run the Device Manager. The PCI-1711 card should show as active in the 'Supported Devices' window. Exit the device manager.

Upgrading and installing downloaded files

This section refers only to the users upgrading the Advantech software. Refer to the previous section for first installation instructions.

The latest version of software can be downloaded from the Advantech website if you have an older version. You will need to download and install both the device driver (Universal 32-bit DLL Drivers V2.2 or higher, PCI1711.exe) and device manager (V2.4 or higher, DevMgr.exe).

Uninstall any previous version of the drivers:

Run Advantech Device Manager, select the PCI-1711 card from the list of supported devices then select Remove. Close Advantech Device Manager.

Uninstall Advantech Device Manager either using uninstall from the Advantech Program Menu entry or from Control Panel - Add/Remove programs.

Navigate to C:\Program Files and delete the Advantech subdirectory and all its contents.

Navigate to C:\windows\system32\drivers and delete ADS1711.sys.

Do NOT reboot the PC.

Now run the device manager installation DevMgr.exe first, then run the device driver installation PCI1711.exe.

Reboot the PC.

The new hardware will be detected. When asked if Windows can connect to Windows Update to search for software select *No, not this time*.



Figure 15 New Hardware Wizard

At the next screen select *install the software automatically*.

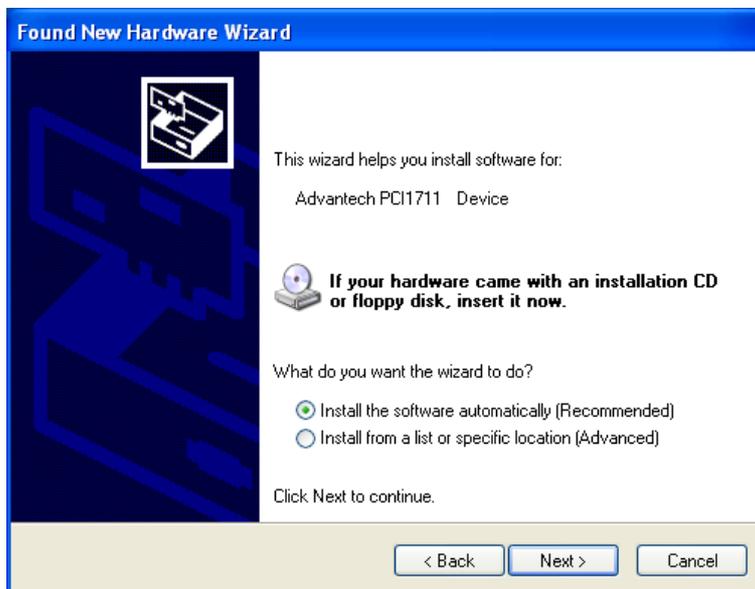


Figure 16 Install New Driver

Windows should find the PCI1711 driver and install it.



Figure 17 Driver Installation Completed

Installation is now complete. To check that the card has installed correctly, navigate from the Start → All Programs menu to Advantech and run the Advantech Device Manager. The PCI-1711 card should show as active in the 'Supported Devices' window. Exit the device manager

Coupled Tanks System software installation

After installing the Advantech software and PCI1711 card you are ready to install the Coupled Tanks software.

1. Close Matlab. Run the setup programme from the CD. The following window will open (Figure 18).

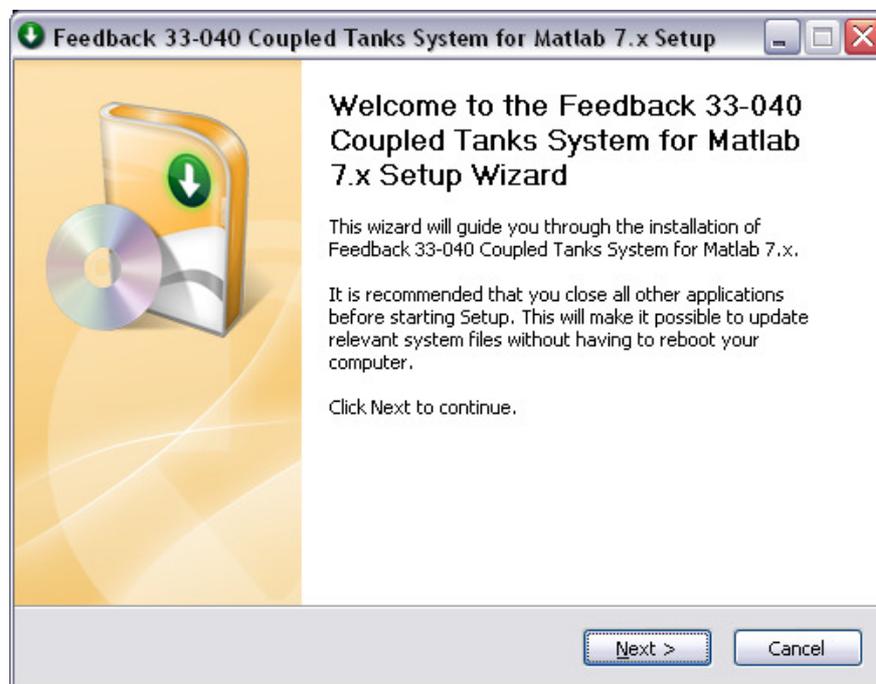


Figure 18 Installation window

2. Click 'Next' to continue. The Matlab version choice window will appear (Figure 19).

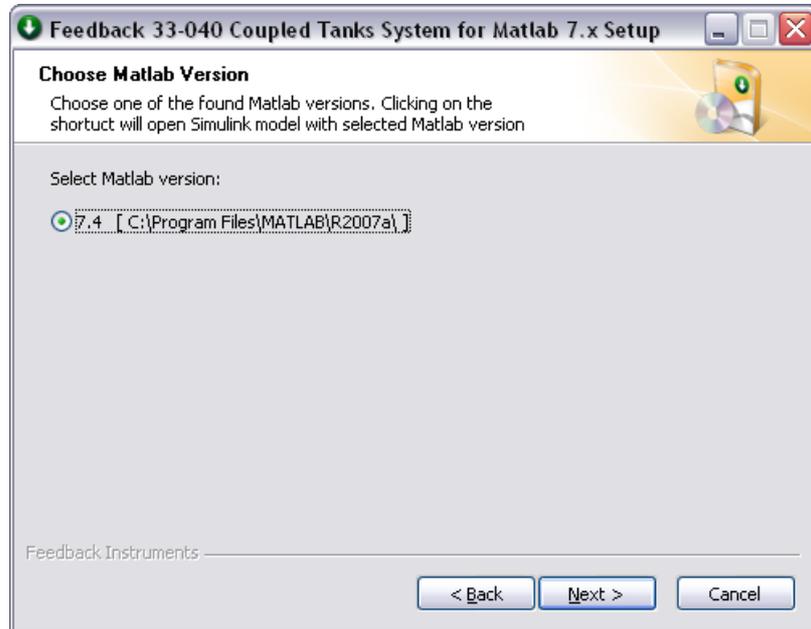


Figure 19 Matlab version choice window

3. Select the Matlab version and click 'Next'. The Installation Destination Folder choice window will appear (Figure 20).

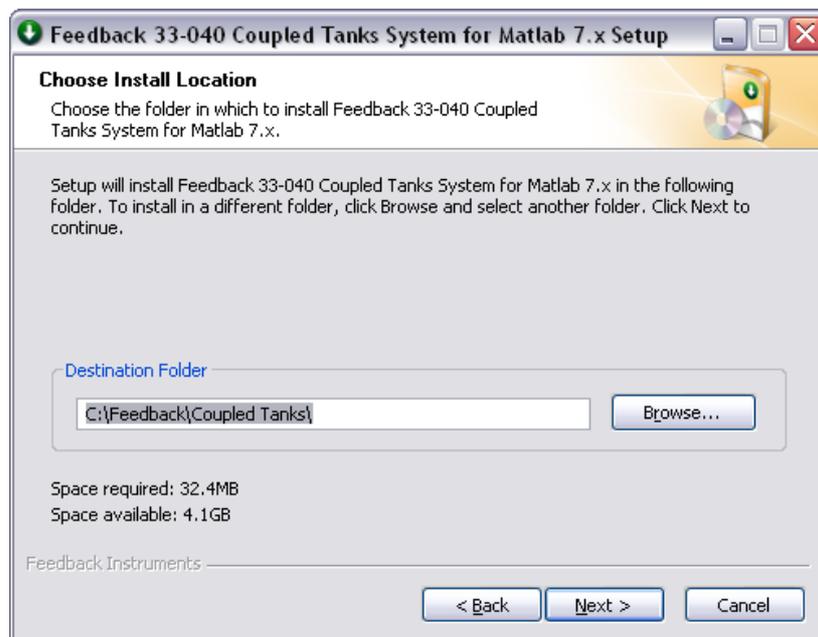


Figure 20 Destination Folder window

COUPLED TANKS SOFTWARE INSTALLATION

4. Select the Destination Folder. Click 'Next' to proceed. The Start Menu Folder window will appear (Figure 21).


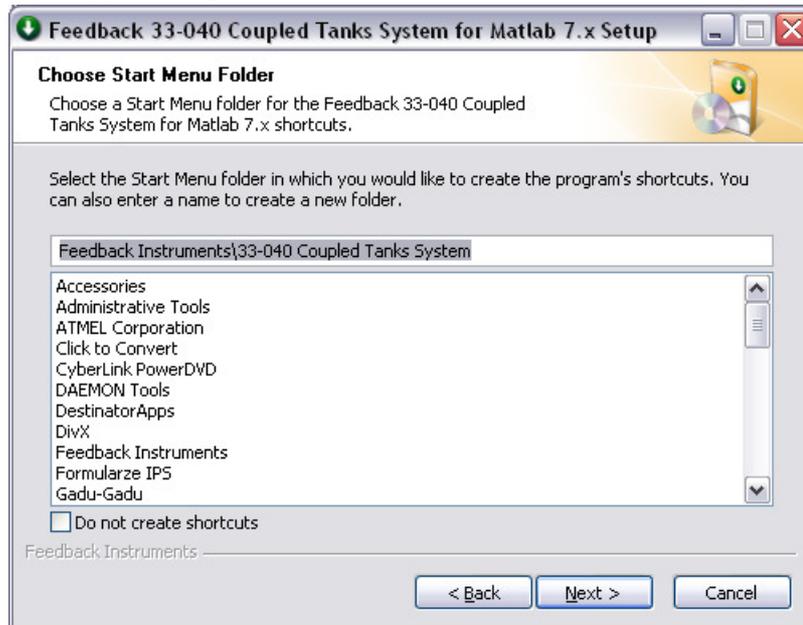


Figure 21 Program Folder window

5. Select the folder to install the project into. Click 'Next' to continue. The Desktop Shortcut option window will appear (Figure 22). Tick to create a desktop shortcut. Press 'Install' to proceed. The Coupled Tanks installer will finish setup with the window presented in Figure 23. Press the 'Finish' button.

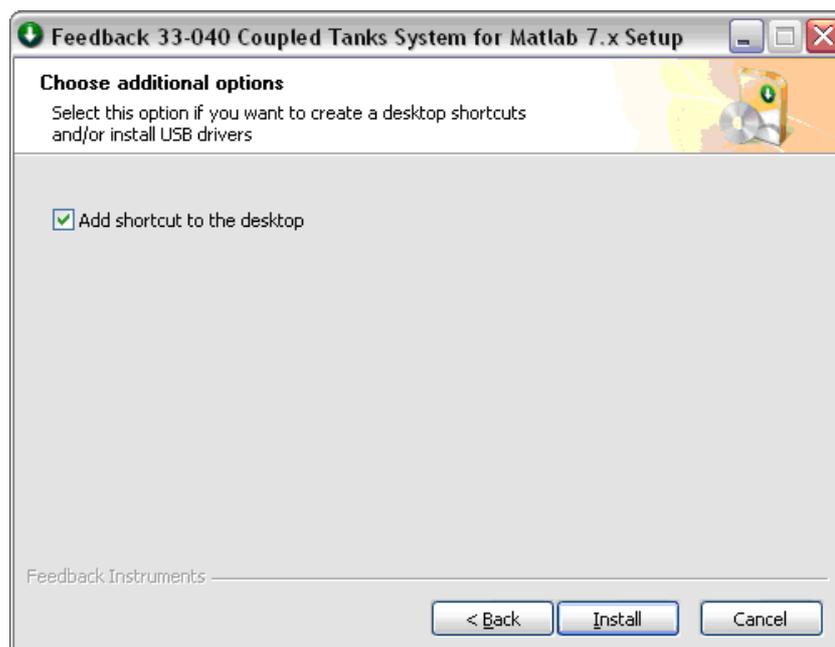

COUPLED TANKS SOFTWARE INSTALLATION

Figure 22 Project installation and USB drivers window

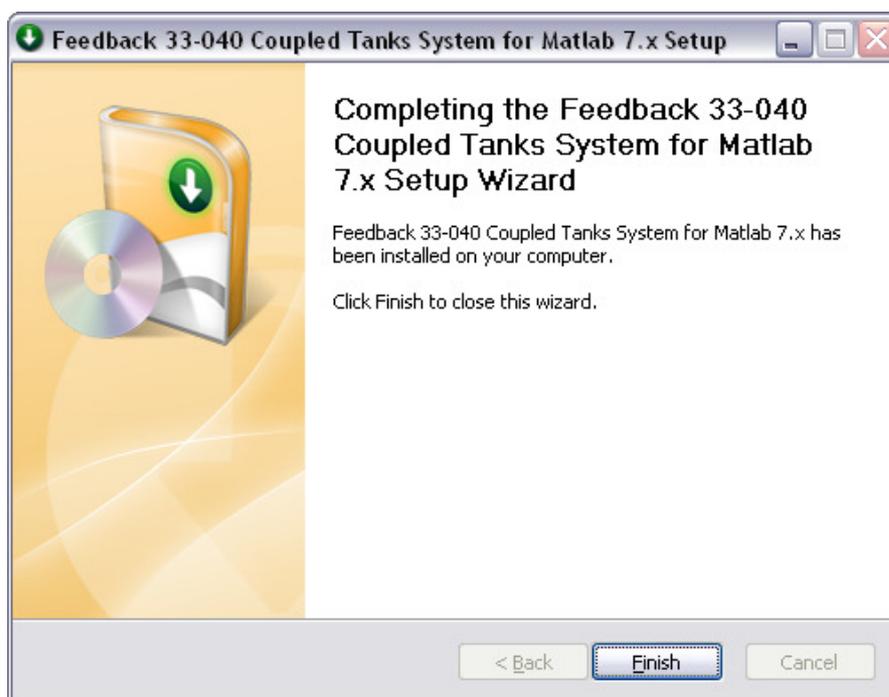


Figure 23 Last installation window

6. Two folders will be available after the installation. 'Real-time models' folder in which the Coupled Tanks Real Time applications are loaded and 'Simulation models' folder in which all of the model simulations files are placed.

PC and Coupled Tanks connection

With all of the software installed you are ready to connect the PC to the hardware. The following elements have to be connected to complete the setup:

1. PC containing the PCI-1711 card
2. Cable connector box
3. Coupled Tanks PSUPA (Power Supply Power Amplifier)

Refer to the connection schematic presented in Figure 24 and follow the steps below.

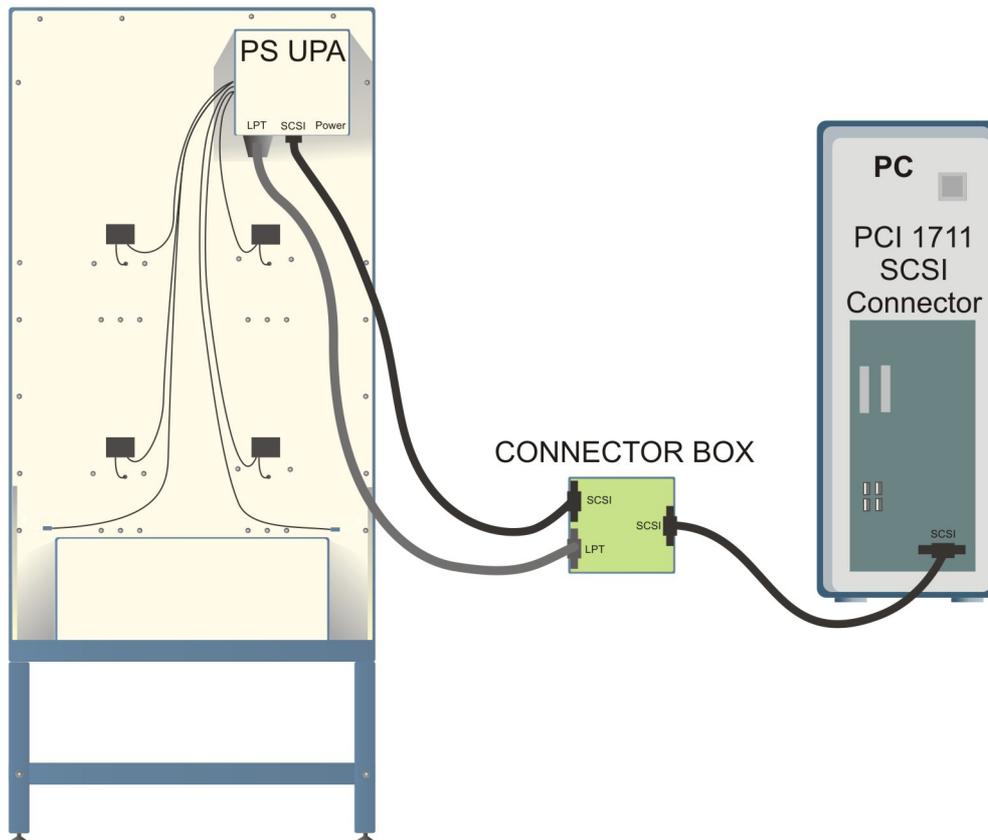


Figure 24 Connection diagram

1. Connect the PCI1711 SCSI Connector to the Feedback Cable Connector Box.
2. Use the 25 way SUB-D connector to connect the Connector Box with the proper SUB-D port of the PSUPA on the Coupled Tanks rig.
3. Connect the mains power cable into the PSUPA and plug it into your mains supply.

Location of Simulink model files

The example Simulink models supplied are stored in two subdirectories. Their location can be selected during installation. The default locations are:

C:\Feedback\Coupled Tanks\Examples\Real-time models

C:\Feedback\Coupled Tanks\Examples\Simulation models

These models can be edited, saved, built etc. as required. A protected copy of the example models has been made so these copies can be used to reinstate the models within the examples directories when required. The default locations of the protected examples are:

C:\Feedback\Coupled Tanks \Example backup\Real-time models

C:\Feedback\Coupled Tanks \Example backup\Simulation models

To reinstate the original models, delete all files within the *Examples\Real-time models* and *Examples\Simulation models* directories and copy in the contents of the *Example backup\Real-time models* and *Example backup\Simulation model* directories respectively.

Load Matlab and the menu system using the Windows Start menu (Figure 25).



Figure 25 Start menu

Matlab will run and the Simulink model menu will open (Figure 26).



Figure 26 Simulink model menu

To run a real-time model for example, double click on the 'Coupled Tanks Real-Time Models' block in the main menu. A sub-menu containing all of the real-time models will open (Figure 27).

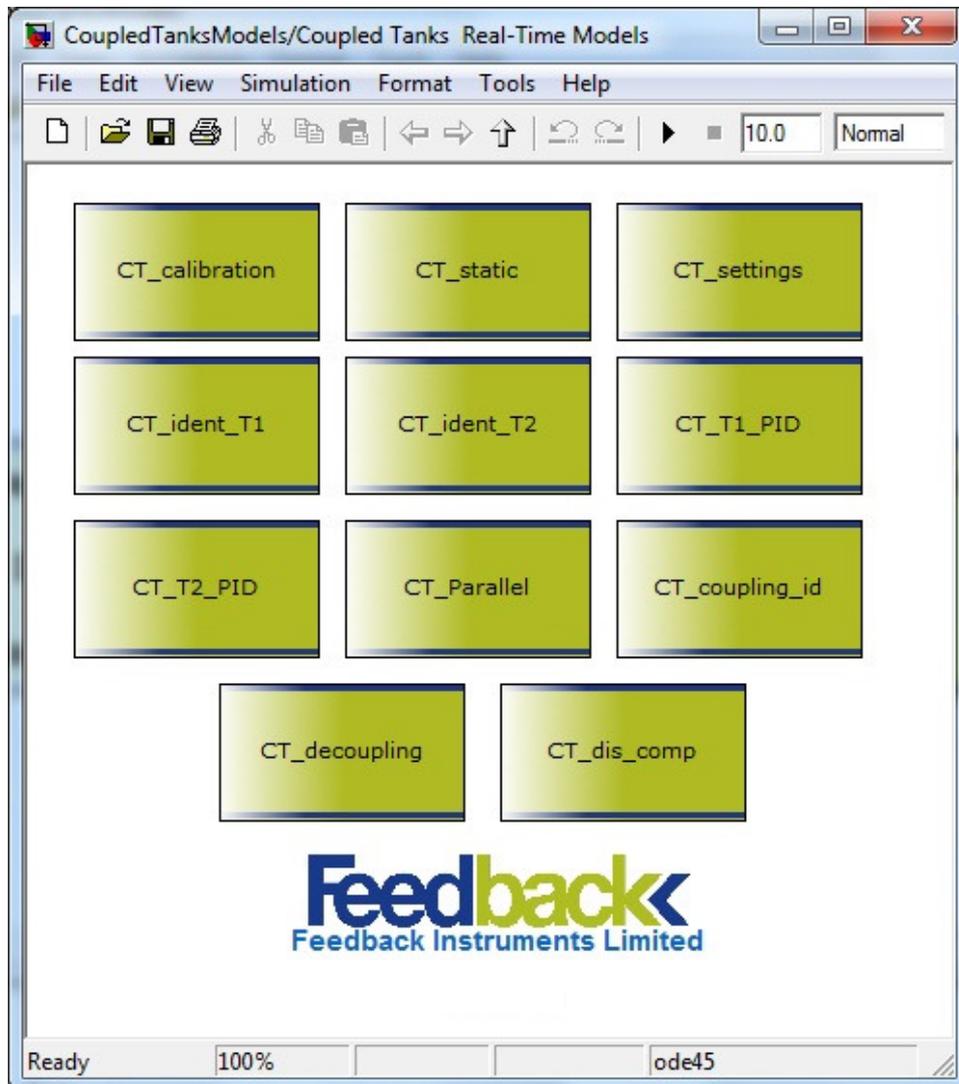


Figure 27 Real-time models menu

Double click the required model, for example *CT_calibration*. The Simulink model window will open Figure 28.

Sensor calibration

Each sensor has to be calibrated before any experiments are run. The calibration should be done periodically to ensure agreement between the real data and the

measured signal. With time passing the water might change its density, which might influence the level reading.

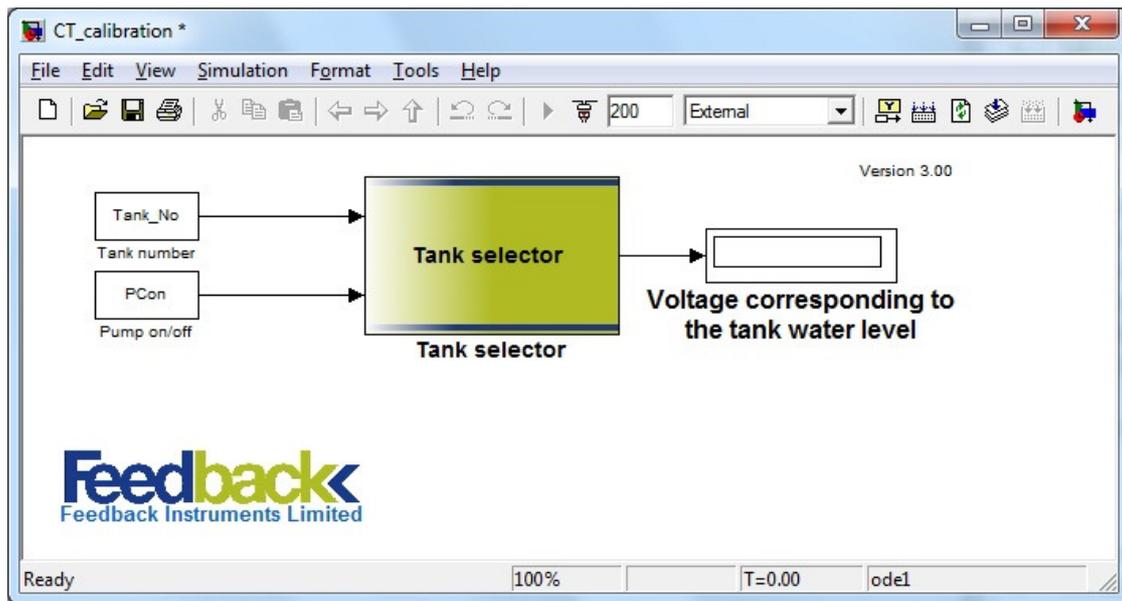


Figure 28 Coupled Tanks calibration window

Follow the instructions below to calibrate the sensors. The sequence has to be repeated for each sensor and tank.

1. Shut the outflow valves of the tank, in which you are going to perform calibration.
2. Open the proper pump output valve (valve **MVB** for tank T1 calibration, valve **MVA** for tank T2 calibration, valve **MVE** for tank T3 calibration, valve **MVD** for tank T4 calibration). Keep the other valves closed, so the water flows directly to the tank, which is being calibrated.
3. Empty the calibrated tank. Place a blocking plastic cap on the outflow pipe so the water cannot run out.
4. Run the *CT_calib.m* file. Follow the given instructions to perform calibration on all of the tanks. The files containing the calibration constants will be saved in the Real-Time models directory.

THE CALIBRATION HAS TO BE PERFORMED BEFORE ANY EXERCISES ARE RUN. CALIBRATION CONSTANTS WILL BE SAVED IN A FILE AND AUTOMATICALLY LOADED WHEN MODELS ARE RUN.

Coupled Tanks Mechanical Unit description

The Coupled Tanks Mechanical Unit consists of 4 tanks attached to the rig. At the bottom of the rig 5th tank is placed for water storage. Inside that tank 2 submersible pumps are placed. The water is pumped up to the top 2 tanks through the series of pipes and configuration valves named 'MV X' ($X = \{A,B,C,D,E,F,G\}$). From the top tanks the water flows freely to the 2 bottom tanks. The orifice size can be varied with 3 cap sizes available, which can be slid on the pipes coming from the bottom of the tanks. With the configuration valves it is possible to introduce coupling between the tanks. The water level can be read in each of the tanks using 4 pressure sensors.

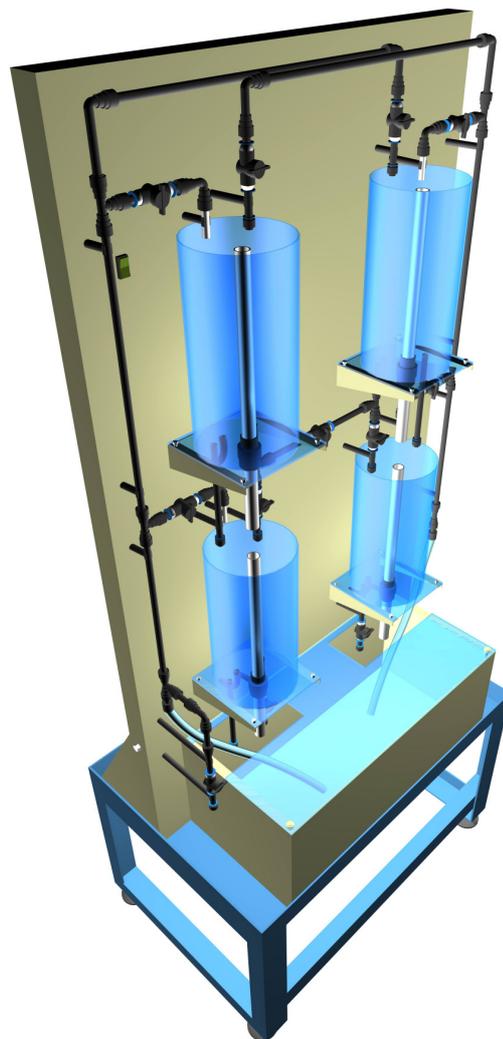


Figure 29 Coupled Tanks Mechanical Unit

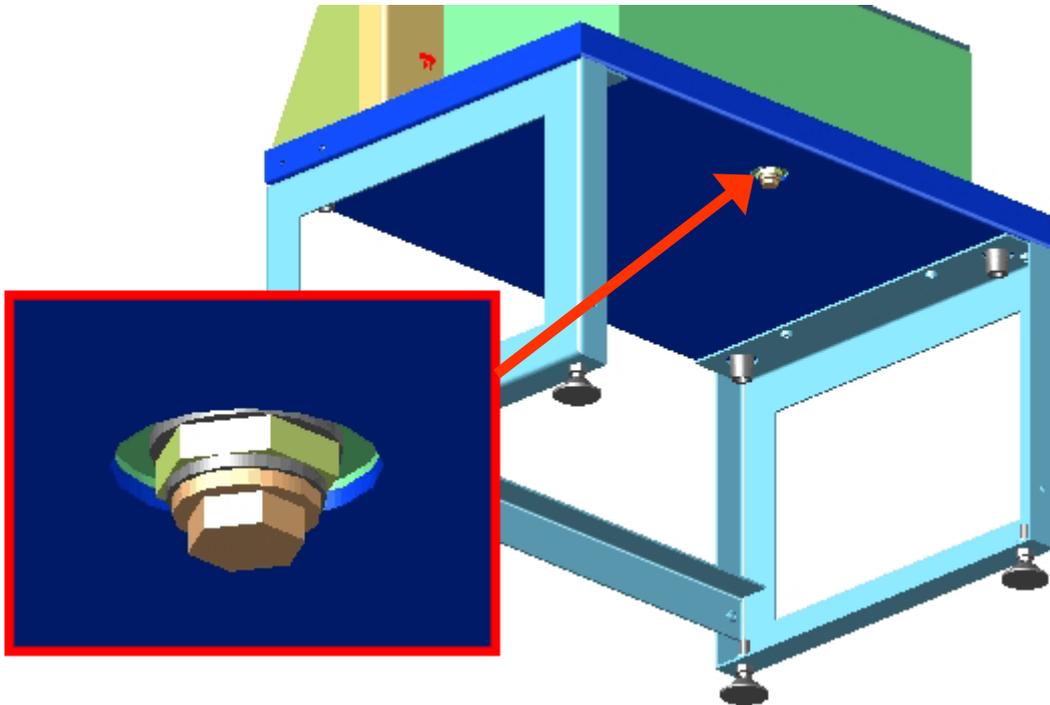


Figure 30 Main tank drain hole

A drain plug is provided at the base of the main tank as shown in Figure 30 which allows water to be fully drained from the system.

It is recommended that as much water as possible is first pumped out of the system via the drain pipe, as follows. The supplied PVC hose should be fitted to the open end of the drain pipe. The system is drained using the left-hand pump only. Valves MV A, MV B and MV C must be closed, the end cap must be removed from the drain pipe, and the drain shut-off valve must be open to allow drainage.

After pumping out as much water as possible, unscrew the nut on the underside of the main tank to empty the residual water from the system into a suitable container. Remember to replace the nut securely and close the drain shut-off valve before filling the system with water again.

WARNING: NEVER ATTEMPT TO TILT THE UNIT WHEN IT CONTAINS WATER.

The unit can be heavy when it contains water. Do not empty the tanks by tilting it. Attempting to do so could be hazardous.

Control system

The Coupled Tanks System is organized according to the schematic presented in Figure 31.

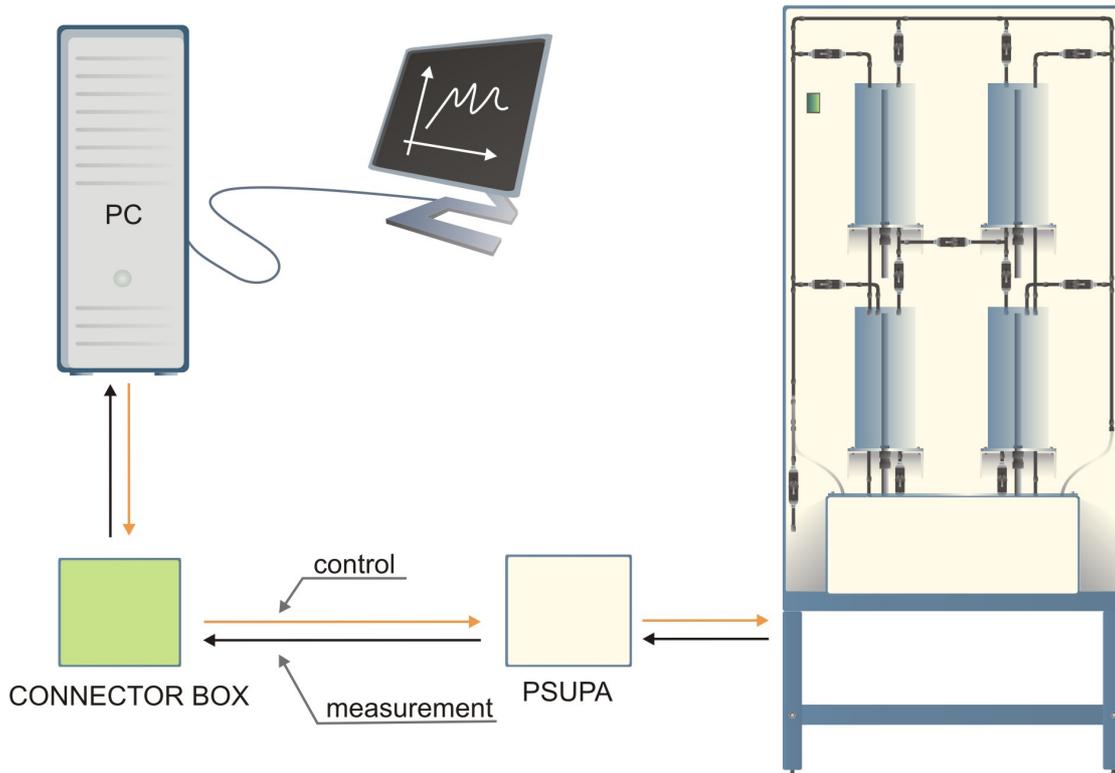


Figure 31 Control system schematic

The PC with Advantech card and Matlab and Simulink environment serve as the main control unit. The control signals, which are voltages between 0 V and 5 V, are transferred to the Power Amplifier where they are transformed into 24 V PWM signals driving the pumps.

The water level in the tanks is measured using pressure sensors. The water level information is transferred to the PC via the PSUPA. From the Simulink point of view the Coupled Tanks (single tank and pump) is seen as the following model presented in Figure 32.



Figure 32 Coupled Tanks model

Computer control

Using MathWorks and Advantech software together simplifies the design of control systems for the Coupled Tanks unit. To design a controller you do not have to build a real-time application from the very beginning. It has been done for you. You can design arbitrary controllers in the Simulink environment and through the Real Time Kernel run them on an external process.

The digital control diagram presented in Figure 33 is used for that purpose.

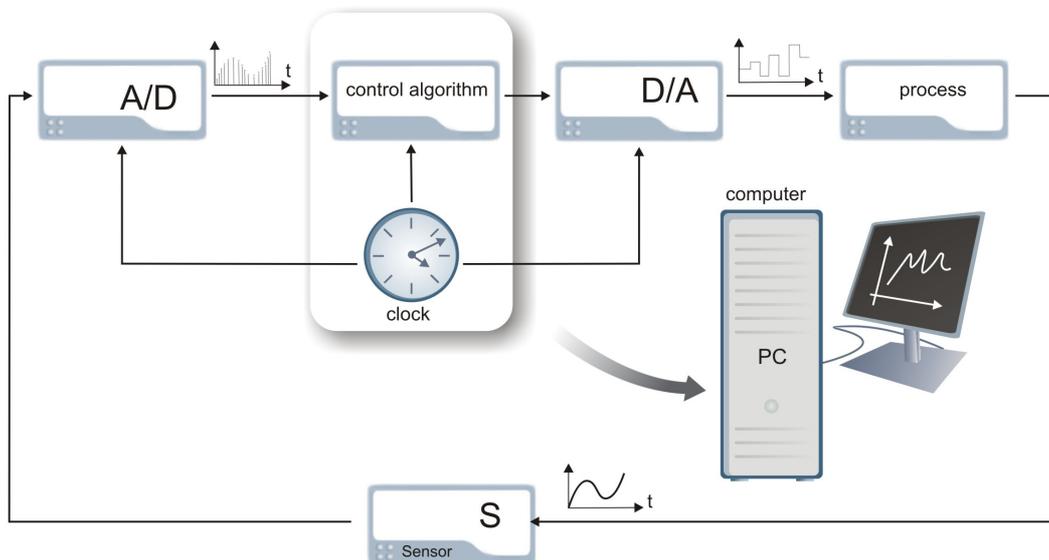


Figure 33 Computer control system diagram

The system consists of four main elements:

1. PC with a clocked control algorithm
2. A/D and D/A converters – serving as an interface between the PC and external environment
3. The controlled process
4. Sensors

The control algorithm and the converters operate according to the time pulses distributed by the clock. The distance between consecutive time pulses is called the sampling time. Usually the sampling time is constant however some special applications use intermittent sampling. The clock delivers an interrupt and an

COMPUTER CONTROL

interrupt service routine (ISR) is called. During the ISR routine an A/D converter delivers a discrete representation of the measurement returned by the sensor. Based on the measurement the control algorithm calculates the value of the control signal. At the end of the ISR the control signal value is updated and set by the D/A converter to be held for the next sampling interval.

The same control scheme is used for the Coupled Tanks system.

Simulink Coupled Tanks control

After software installation two folders are created, which contain Simulink files. One of them contains files for simulation; the second folder contains files for real-time Coupled Tanks control.

The simulation only files can be used as normal Simulink experiments.

Real-time control

Real time control applications refer to an external source (external equipment). In Figure 34 an example position control application is presented.

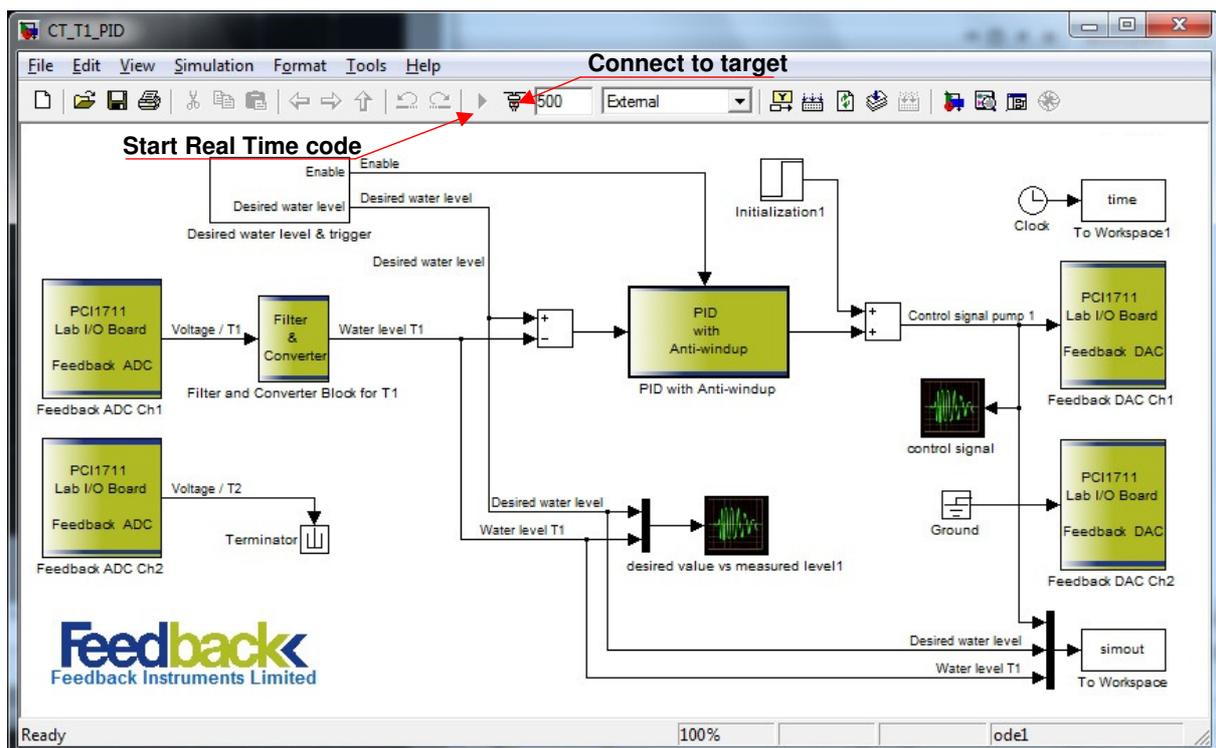


Figure 34 PID Tank1 water level control

The models can be run by navigating using either the Windows *start* menu:

Start menu → All Programs → Feedback Instruments → Feedback 33-041.. → Simulink Models

and category choice (Figure 35)

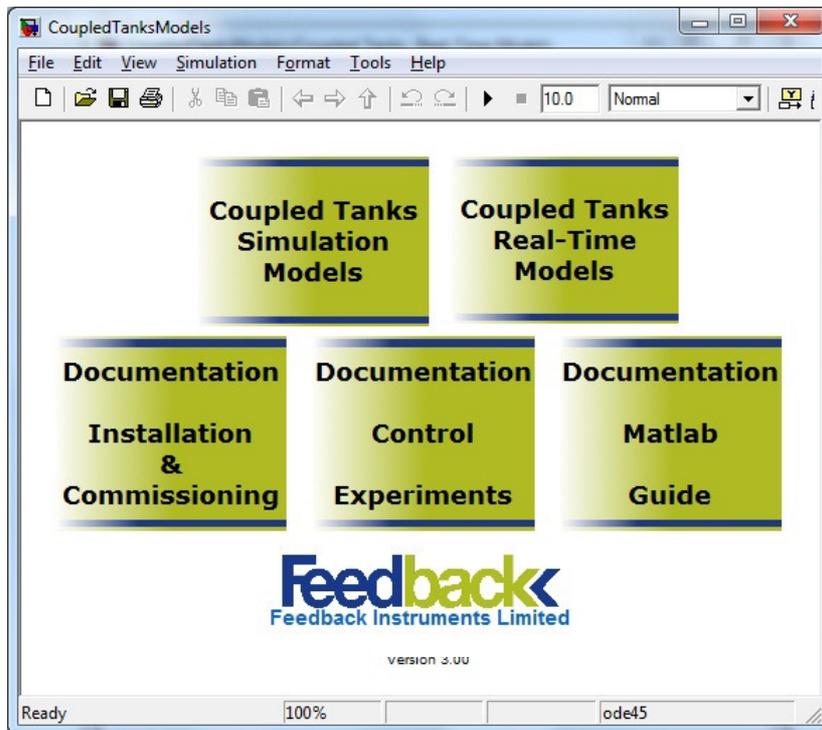


Figure 35 Model category window

or by loading Matlab then using the following path:

C:\Feedback\Coupled Tanks\Examples\Real-time models\

If you have two Matlab installations available, make sure that the Coupled Tanks software is installed for the Matlab that you want to use for Coupled Tanks. If it is the first time you are running real-time experiments on that version of Matlab type the:

rtwintgt -setup

command and execute it in Matlab.

When 'CT_T1_PID' is selected the model presented in Figure 34 will open. The simulation parameters are already set. If you want to make your own applications you have to use the same simulation parameters like solver options for example. Thus it is easier to use one of the existing applications and modifying it according to your needs without changing the simulation parameters.

SIMULINK COUPLED TANKS CONTROL

NOTE: The reservoir tank should be full with the pumps fully submersed in water. Make sure that the unit is calibrated and that static characteristic and working point is identified (see Control Experiments manual).

Connect the application with the PCI1711 card by pressing the CONNECT TO TARGET button (Figure 37). The application will not run yet. Now turn the Coupled Tanks power on.

You can start the application by pressing the START REAL TIME CODE button (Figure 34).

More information on 'CT_T1_PID.mdl' is given in the 'Control Experiments' manual.

New controllers design

It is best to start your own controller design by using the already made application and removing its content apart from two important blocks (Figure 36), which are the 'Feedback ADC block' and the 'Feedback DAC block' and Feedback logo block. This way all of the simulation parameters that are needed for the Real Time application will be set.

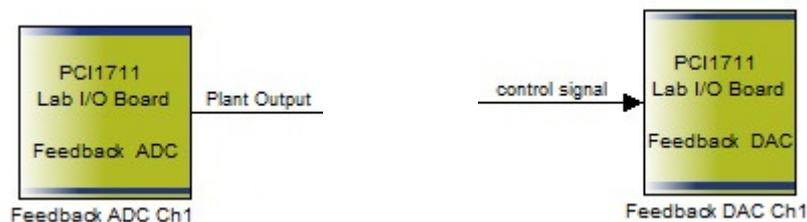


Figure 36 External equipment blocks

The 'Feedback ADC block' has one output, which is the voltage corresponding to the water level in the tank. You do not need to modify these blocks. Modifications may cause serious problems with control applications. The 'Feedback DAC' block has one input, which is the control voltage.

It is best if you start with existing control applications parameters' modifications or design very simple algorithms to get familiar with the Coupled Tanks setup.

PCI 1711 Lab I/O Block – Feedback DAC

- This is a universal Feedback block which sends the input value to *PCI-1711 analog output*.
- There is one input in this block and the block reads the value from this input and sends it to the analogue output of the PCI-1711 card (Figure 37).

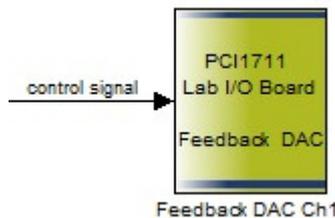


Figure 37 Feedback DAC Block – one input

- There are two parameters available: sample time and output channel. We can choose between 1 or 2 for output channels. This is because *PCI-1711 analog output* contains two channels.
- By double clicking on this block we can change the above parameters (Figure 38).

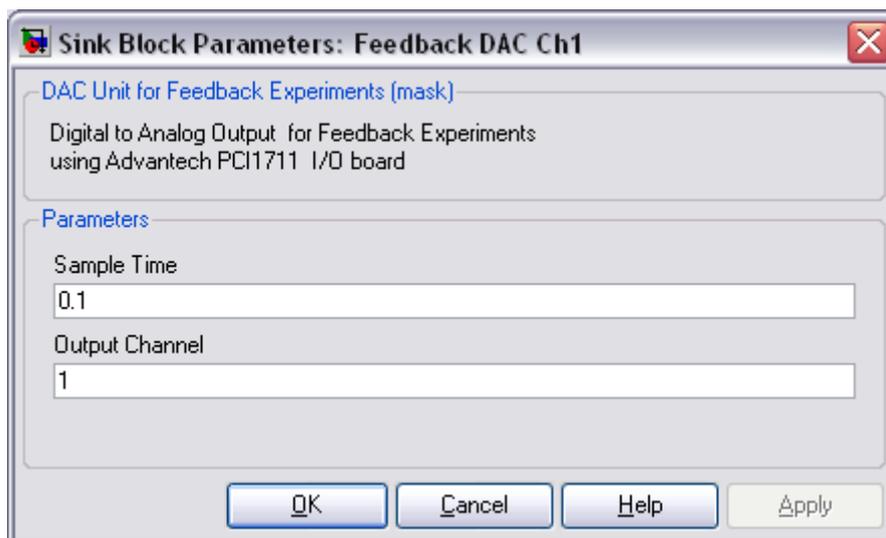


Figure 38 Feedback DAC Block – parameters

- The value, which is sent to the analogue output is the accepted range of 0V to 5V.
- Choose “*Look under Mask*” to view all of the subsystems (Figure 39). Before any experiments are run the PCI-1711 card has to be registered and set up. Double click on the Analog Output block and register the PCI-1711 card in Matlab environment (Figure 40).

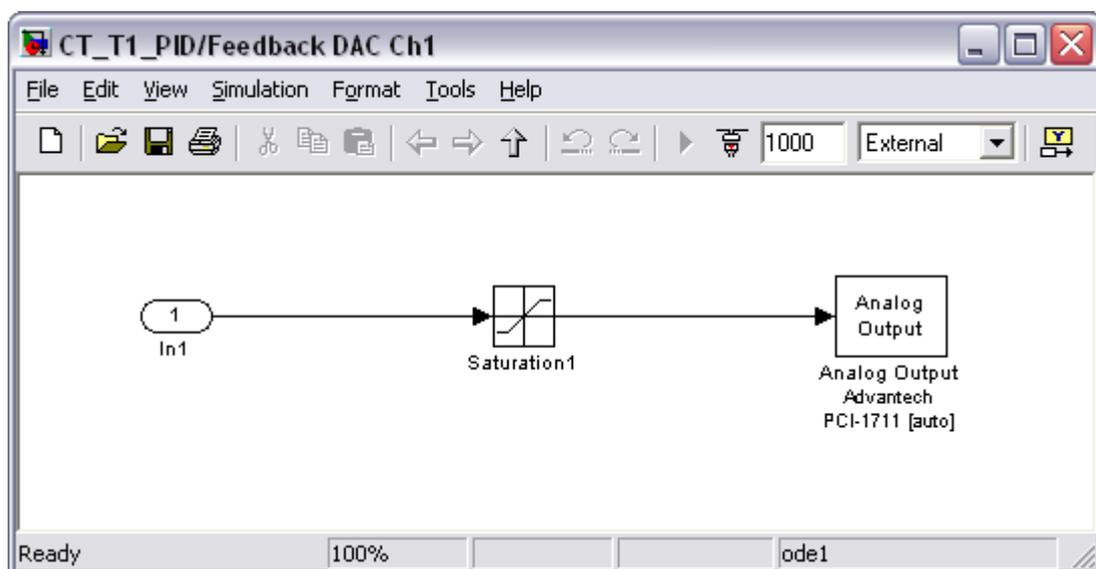


Figure 39 Feedback DAC Block –under mask

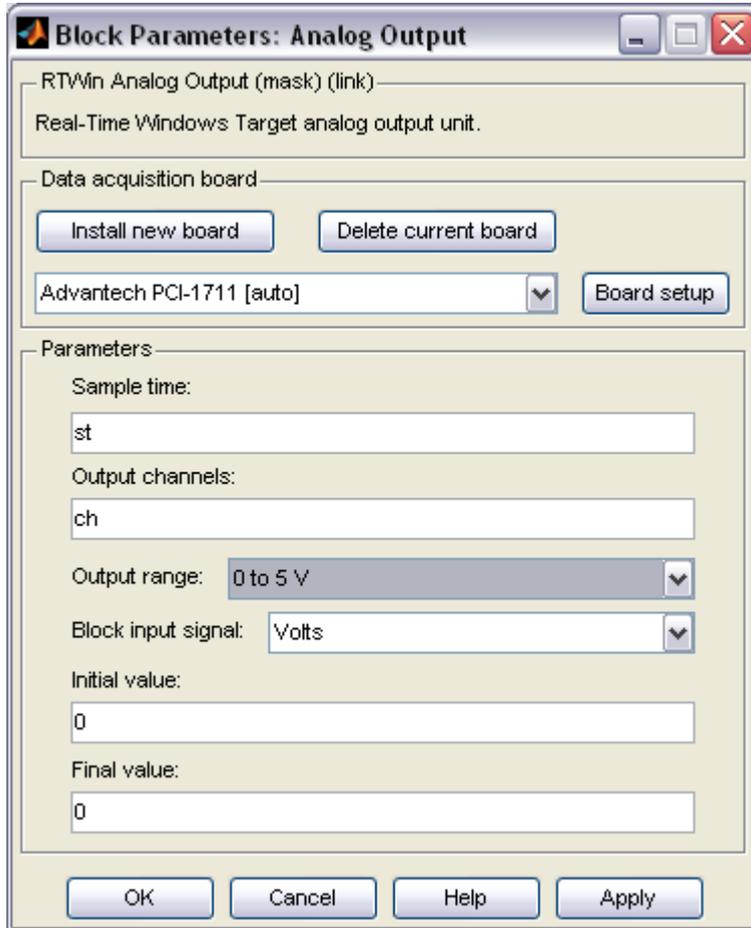


Figure 40 Feedback DAC Block – board setup